


Cannulation Pack



Trust policy that Bionector is attached to **ALL** cannulae.

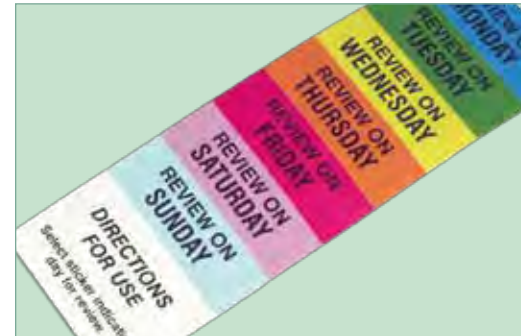

Please ensure **ALL** paperwork is completed before leaving the patients' bedside.



Clean Bionector before use and wait 30 seconds.



Please ensure **ALL** contents of the pack are used when cannulating to ensure best practice.

For further information please contact your Vygon Sales Executive, *****

t: ***** e: *****