




V-Green Spinal Needles

Part of Vygon's Regional Anaesthesia Product Range

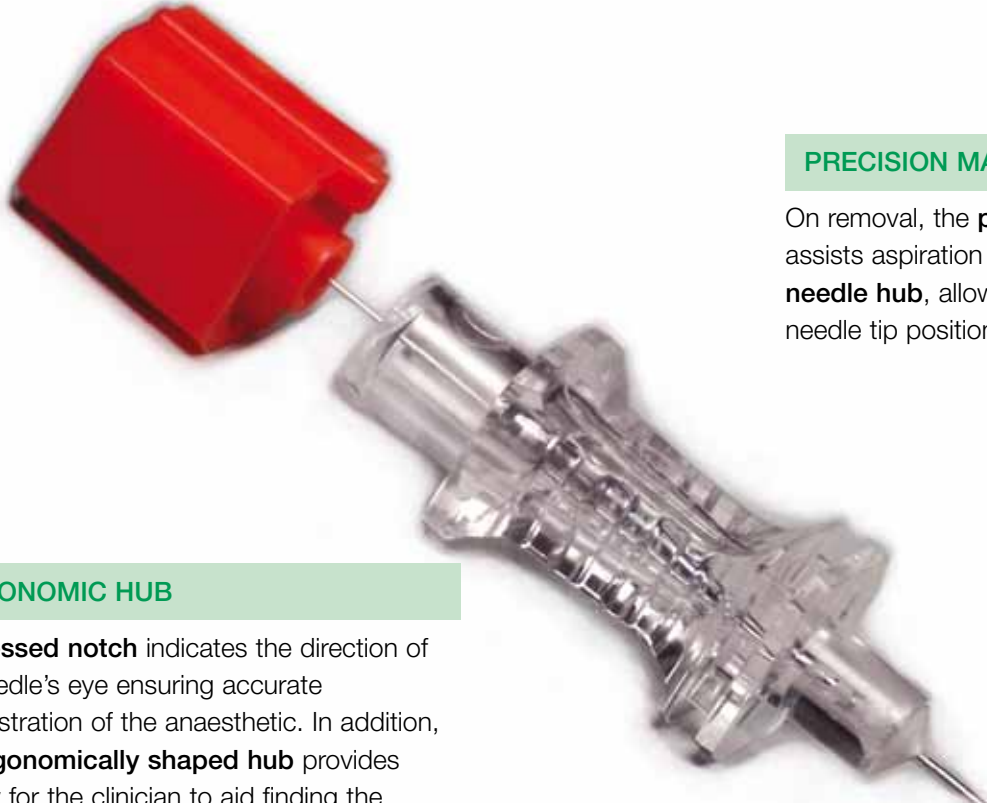

PRECISION MATCHED STYLET

On removal, the **precision matched stylet** assists aspiration of CSF into the **clear needle hub**, allowing quick recognition of needle tip position.

ERGONOMIC HUB

A **recessed notch** indicates the direction of the needle's eye ensuring accurate administration of the anaesthetic. In addition, the **ergonomically shaped hub** provides tactility for the clinician to aid finding the spinal space more easily.

WHITACRE PENCIL POINT DESIGN

In addition to reducing the risk of post spinal headache the **small lateral eye** prevents the injectate being delivered into both the epidural and intrathecal space, resulting in a partial block.




PLASTIC HUB INTRODUCER

V-Green spinal needles include an introducer with an **ergonomic plastic hub**, which provides stability and aids smooth unimpeded insertion of the spinal needle.

ORDERING DETAILS

Vygon Code	NPC Code	Gauge	Needle		Colour	Introducer		Box Quantity	✓
			Size (mm)	Length (mm)		Gauge (mm)	Length (mm)		
0181.052	FTR592	25	0.50	90	Orange	20	38	20	
0181.252	FTR591	25	0.50	120	Orange	20	38	20	
0181.452	FTR593	25	0.50	145	Orange	20	38	20	
0181.442	FTR588	27	0.40	38	Grey	22	38	20	
0181.042	FTR587	27	0.40	90	Grey	22	38	20	
0181.242	FTR590	27	0.40	120	Grey	22	38	20	
0181.07	FTR188	22	0.70	90	Black	-	-	20	
5181.27	FTR241	22	0.70	120	Black	-	-	20	

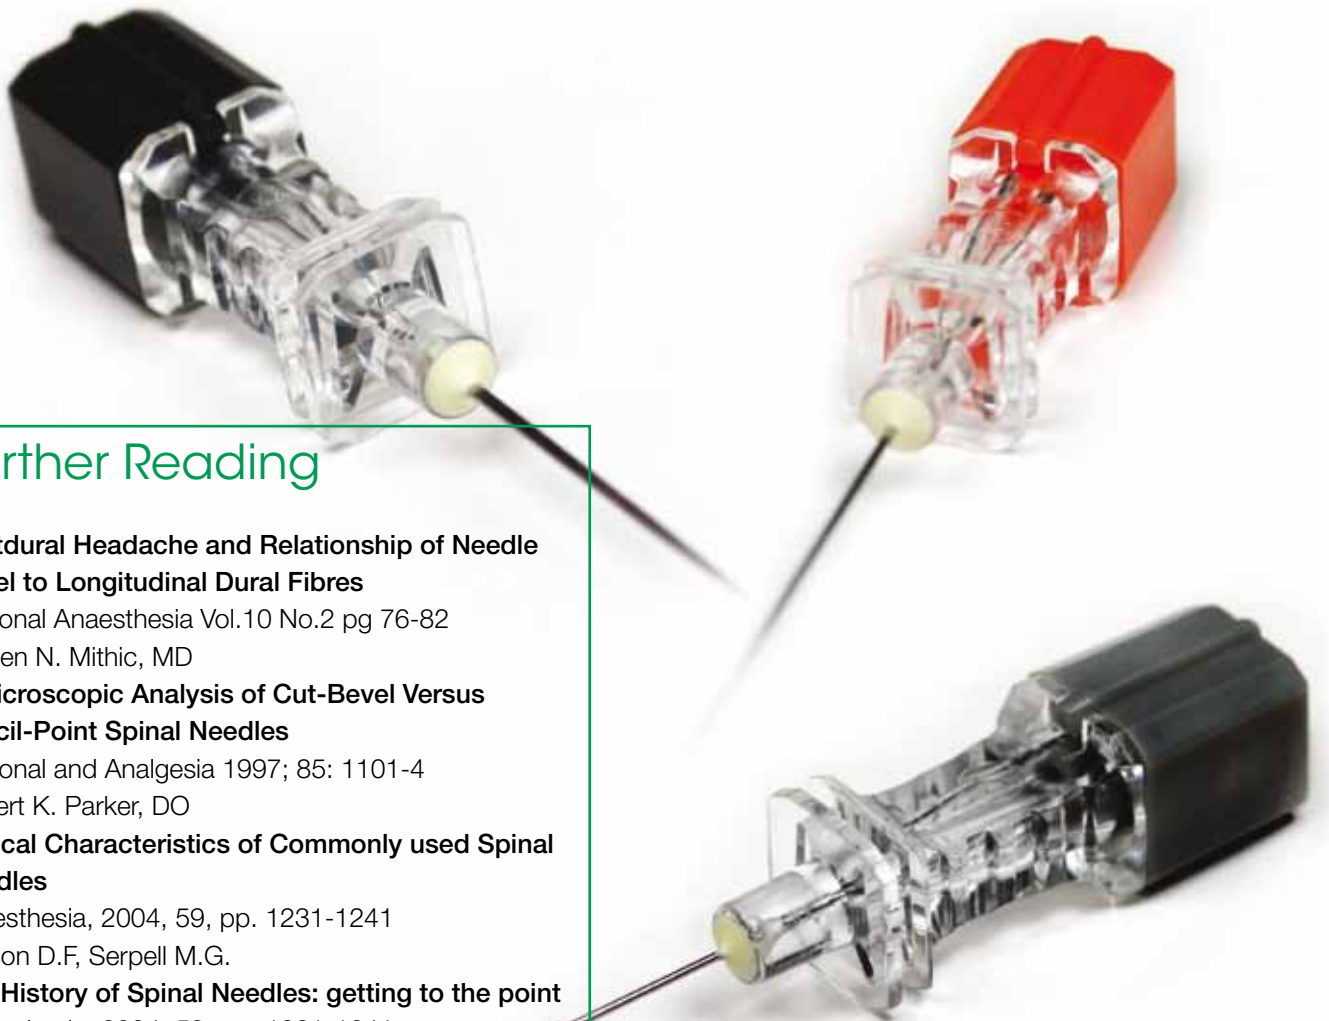

Further Reading

Postdural Headache and Relationship of Needle Bevel to Longitudinal Dural Fibres

Regional Anaesthesia Vol.10 No.2 pg 76-82

Drazen N. Mithic, MD

A Microscopic Analysis of Cut-Bevel Versus Pencil-Point Spinal Needles

Regional and Analgesia 1997; 85: 1101-4

Robert K. Parker, DO

Clinical Characteristics of Commonly used Spinal Needles

Anaesthesia, 2004, 59, pp. 1231-1241

Carson D.F, Serpell M.G.

The History of Spinal Needles: getting to the point

Anaesthesia, 2004, 59, pp. 1231-1241

N. Calthrope

Postdural Puncture Headache (PDPH) : Onset, Duration, Severity, and Associated Symptoms

Acta Anaesthesiol Scand. 1995; 39: 605-612

H.Lybecker



ISO 14001
Produced at a mill that holds
ISO 14001 certification

This brochure has been printed using environmentally-friendly processes, on paper from well-managed sources, and can be recycled. If you would like to receive an electronic copy, please contact the Vygon Customer Services team on 01285 657051.



Vygon (UK) Ltd,

Web: www.vygon.co.uk Email: vygon@vygon.co.uk - Content correct as of 12/08 - Code: 0035.V-GREENSP